

3M™ Curosu Jet™ Disinfecting Cap for Needleless Connectors

Hates dirty. Loves clean

Curosu Jet Disinfecting Caps are the next-generation solution for needleless connector disinfection. Meeting the high-efficacy standards of all Curosu devices, Curosu Jet disinfecting caps utilize a spray of 70% isopropyl alcohol (IPA) to disinfect all critical surfaces of needleless connectors.

Curosu Jet disinfecting caps are intended for use on needleless connectors as a disinfecting cleaner prior to line access. The device will disinfect the connector one minute after application and protect from contamination between accesses for up to seven days if not removed.

To disinfect any needleless connector, just peel the foil strip from the Curosu Jet disinfecting cap and twist it on.

Disinfects in 1 minute
Protects ports
for up to 7 days

Improved fit

Curosu Jet disinfecting caps twist on easily and stay securely in place on commonly used needleless connectors, including the uniquely threaded Smartsite® needle-free valve.

Easier to handle

A high profile makes the Curosu Jet disinfecting cap easy to handle when wearing gloves.

Convenient dispensing

Curosu Jet disinfecting caps are dispensed as individual caps or on a convenient five-cap strip which can be hung from I.V. poles for easy access.

Designed for patient comfort


Curosu Jet disinfecting caps' rounded edges may improve patient comfort.

Colored bright to disinfect right


Curosu Jet disinfecting caps are brightly colored, making it easy to verify that a port is clean at a glance. Disinfection compliance can be easily and reliably measured.




When twisted onto a needleless connector, Curosu Jet disinfecting caps actively spray IPA.



Unengaged



Engaged:
IPA released

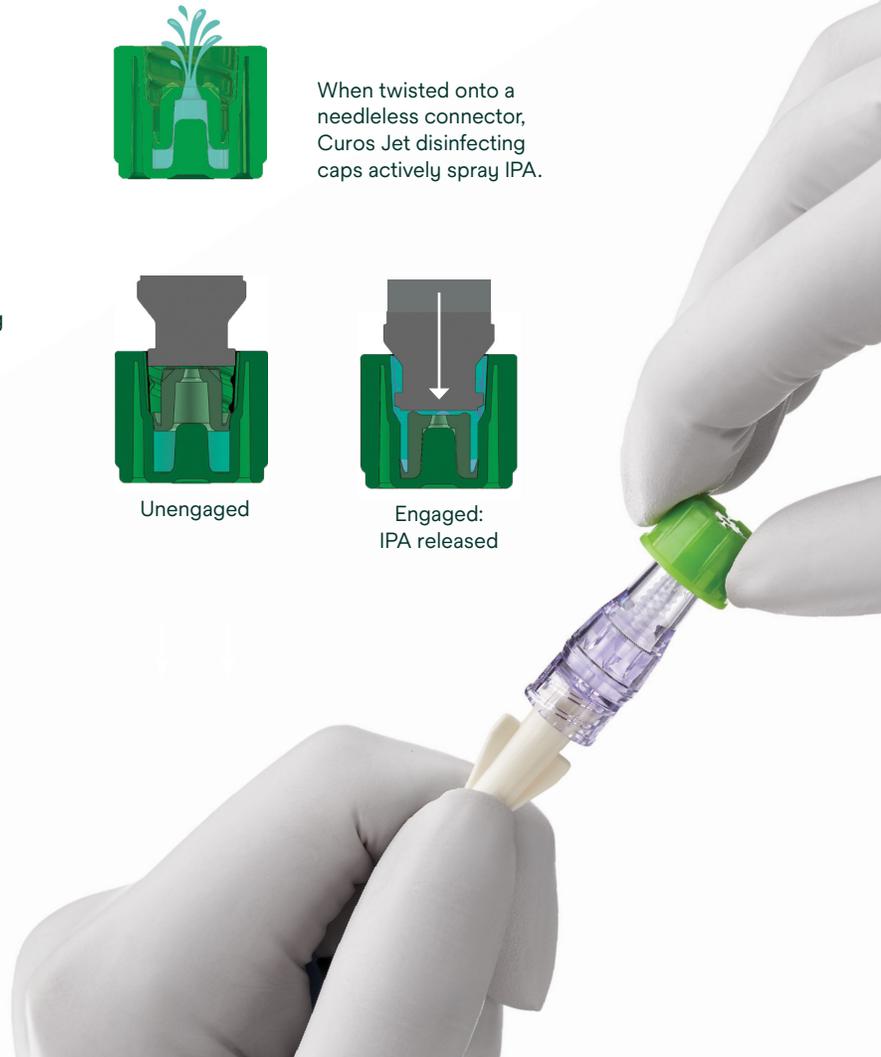

3M™ Curoso™ Disinfecting Port Protectors achieved a 99.99% reduction in 6 microbes commonly associated with CLABSI

The effectiveness of Curoso products was tested *in vitro* against^{1,2}:



Staphylococcus aureus



Staphylococcus epidermidis



Escherichia coli



Candida albicans



Pseudomonas aeruginosa




Candida glabrata

Study conclusion:

All test samples exceeded the minimum 4-log reduction after one minute.

Studies were conducted at independent laboratories. Data on file

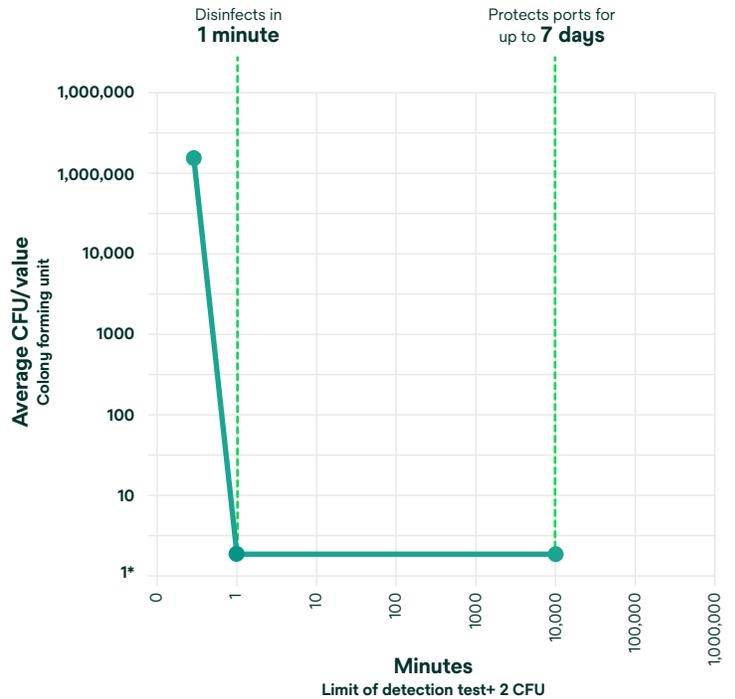

1. For more information regarding organisms associated with catheter-related bloodstream infections, refer to Wenzel RP and Edmond MB. The Impact of Hospital-Acquired Bloodstream Infections. Emerg Infect Dis. 2001 Mar Apr;7(2):174-7.

2. Data reflects *in vitro* findings on Curoso Disinfecting Port Protectors conducted by an independent laboratory.

To order call 800-228-3957

Product	Dispenser	Legacy product order #	Solventum product order #	Boxes per case	Units per box	Total caps per case
Curoso Jet Disinfecting Caps	Individuals	—	CFJ1-270	20	270	5,400
	Strips (5 count)	006-250-5	CFJ5-250	20	50 Strips	5,000



Solventum Medical Surgical

Phone 800-228-3957

Web go.Solventum.com/curoso

© Solventum 2025. Solventum, the S logo and other trademarks are trademarks of Solventum or its affiliates. 3M, the 3M logo and other trademarks are trademarks of 3M. Other trademarks are the property of their respective owners.

70-2011-5719-8